


Report Title


Test Name:	BCR-ABL Universal	Test Sample:	BCR-ABL-Major
Test Time:	2025-12-23 17:18:14	Report Time:	2025-12-25

Well	Dyes	Targets	Name	Type	Ct	Result-1	Result-2	Final Result
B2	FAM	Major	BCR-ABL-Major	STD	15.42	Positive	Positive	Positive
	NONE							
	TEXAS RED	ABL			16.13	Positive		
	NONE							
	NONE							
	NONE							
B3	FAM	Major	BCR-ABL-Major	STD	18.94	Positive	Positive	Positive
	NONE							
	TEXAS RED	ABL			19.01	Positive		
	NONE							
	NONE							
	NONE							
B4	FAM	Major	BCR-ABL-Major	STD	22.74	Positive	Positive	Positive
	NONE							
	TEXAS RED	ABL			22.41	Positive		
	NONE							
	NONE							
	NONE							
B5	FAM	Major	BCR-ABL-Major	STD	26.20	Positive	Positive	Positive
	NONE							
	TEXAS RED	ABL			25.96	Positive		
	NONE							
	NONE							
	NONE							
B6	FAM	Major	BCR-ABL-Major	STD	28.75	Positive	Positive	Positive
	NONE							
	TEXAS RED	ABL			28.85	Positive		
	NONE							
	NONE							
	NONE							

RFU

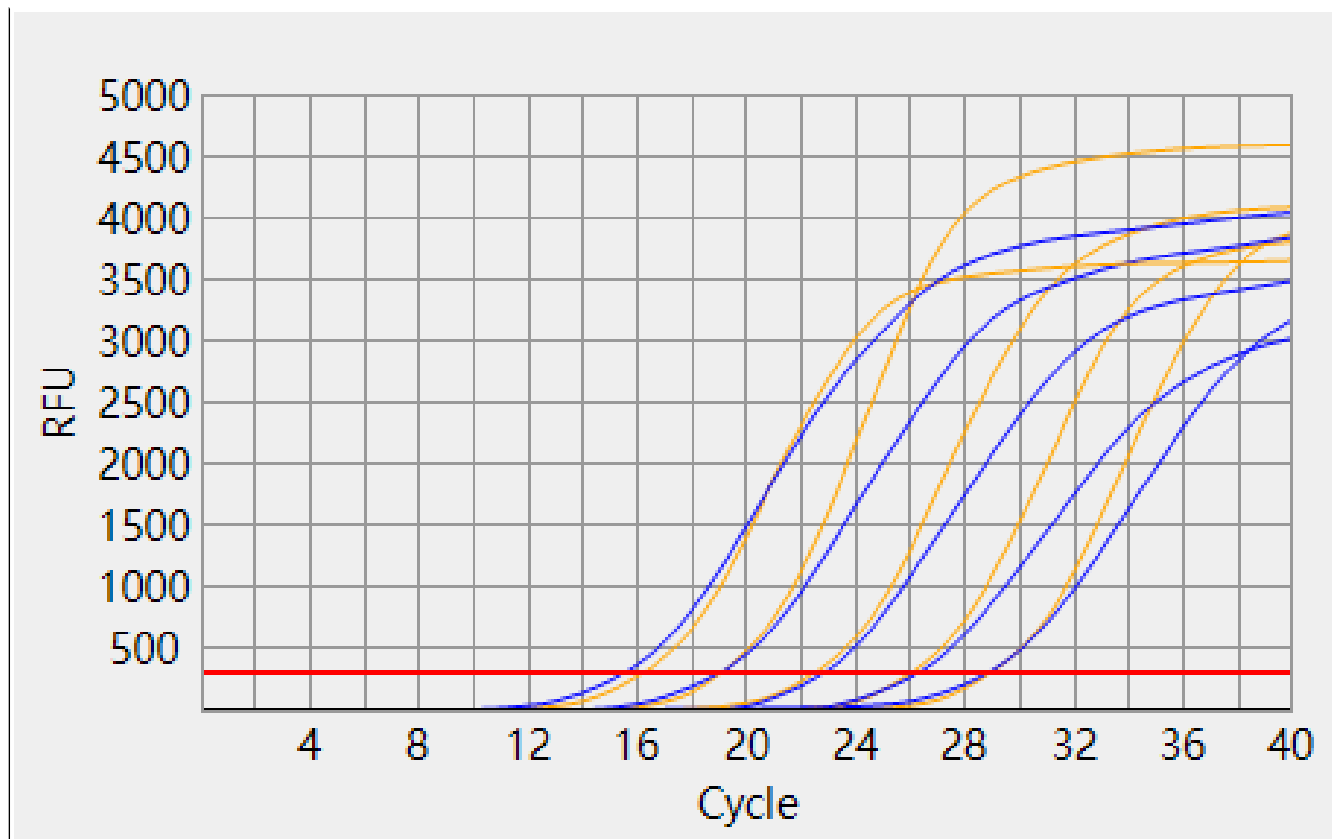

When the Ct value of the sample to be tested is outside the reference range and there is a typical S-shaped amplification curve, the test result is positive;
 When the Ct value of the sample to be tested is within the reference range, or the Ct value is outside the reference range but there is no typical S-shaped amplification curve, the test result is negative.

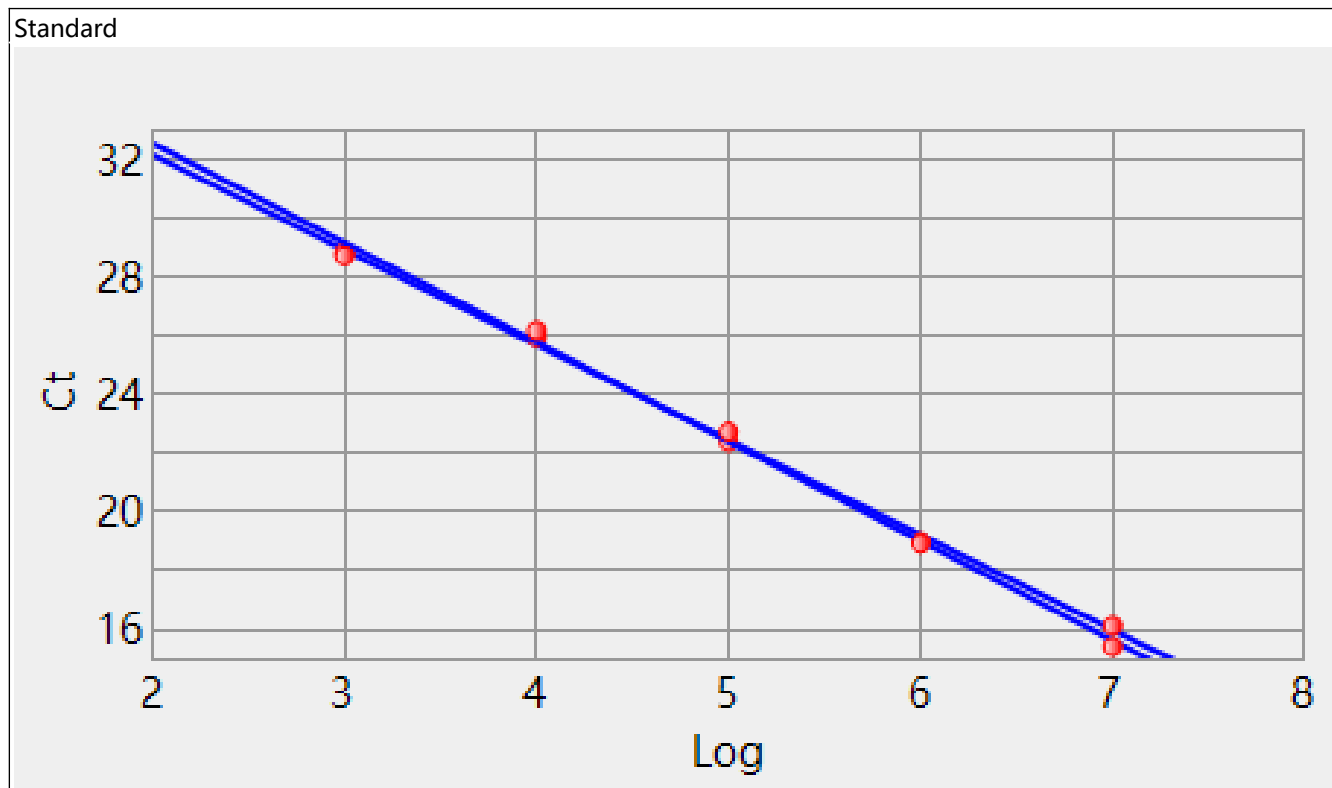

Channel 1 Slope: -3.392 Intercept: 39.372 Correlation: -0.998 Efficiency3: 97.1430
 Channel 3 Slope: -3.240 Intercept: 38.672 Correlation: -0.999 Efficiency2: 103.52