


# Report Title

Test Name:	MTC-Q	Test Sample:	MTC-3
Test Time:	2025-04-23 10:16:34	Report Time:	2025-12-25

Well	Dyes	Targets	Name	Type	Ct	Result-1	Result-2	Final Result
C1	FAM	IS6110	MTC-3	PC	18.92	Positive	Positive	Positive
	HEX	IC			18.58	Negative		
	TEXAS RED	mpt64			19.32	Positive		
	NONE							
	NONE							
	NONE							

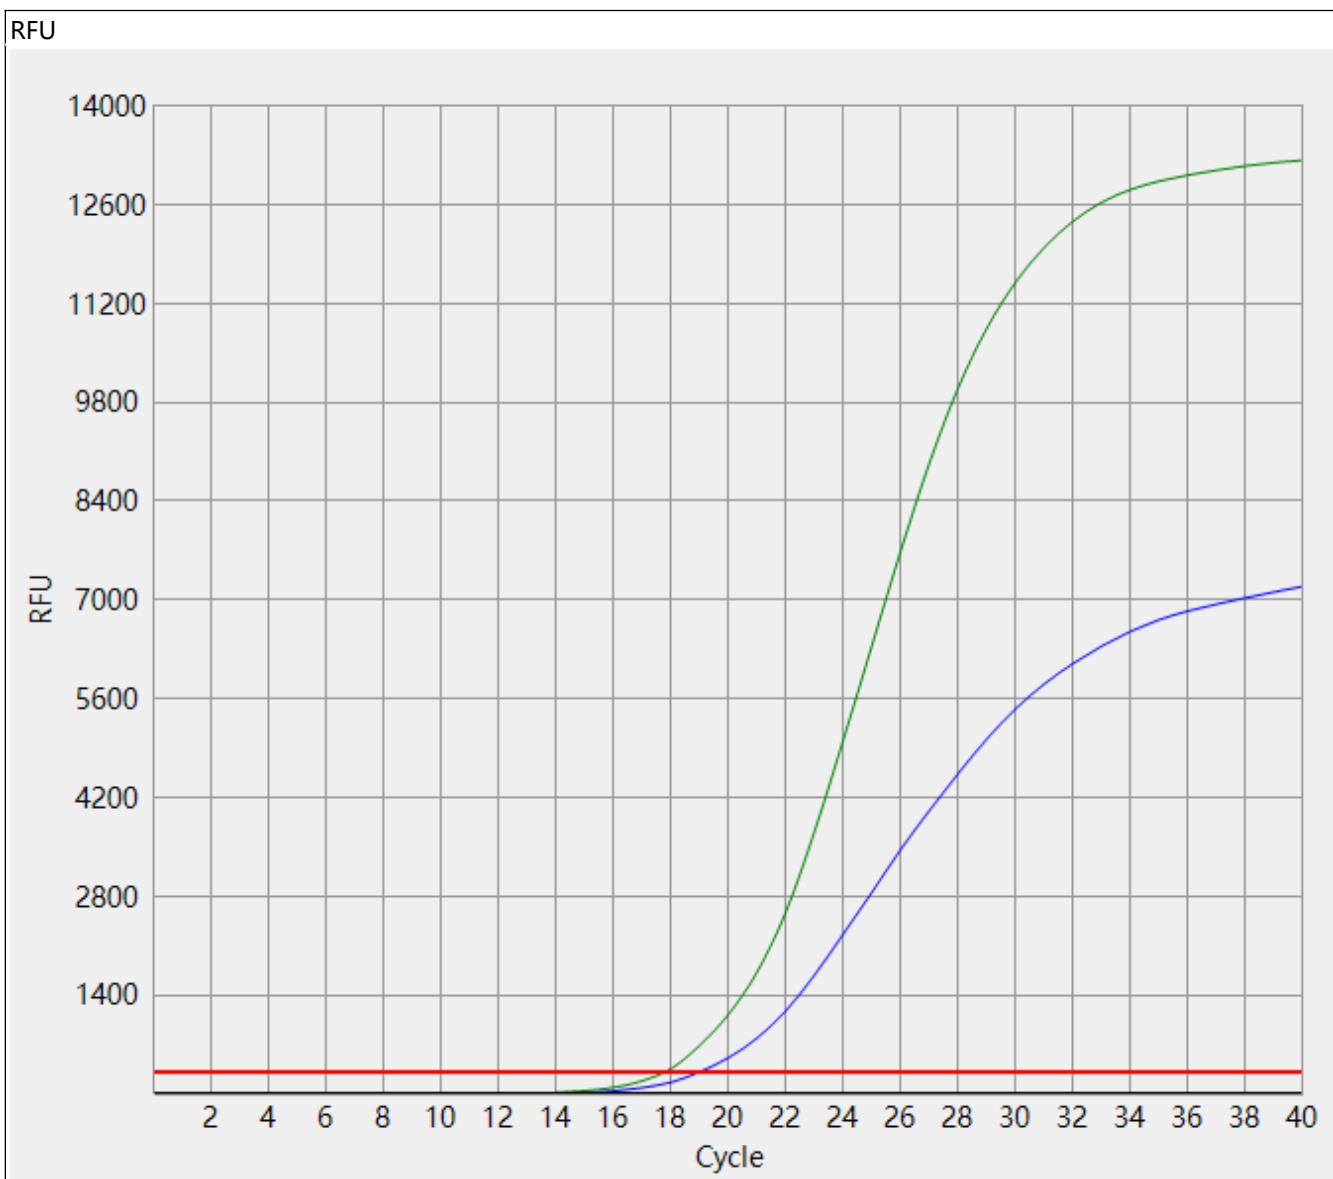

When the Ct value of the sample to be tested is outside the reference range and there is a typical S-shaped amplification curve, the test result is positive;

When the Ct value of the sample to be tested is within the reference range, or the Ct value is outside the reference range but there is no typical S-shaped amplification curve, the test result is negative.